



NC-VP-PBS

Nurse Call Patient Bed Station Vandal Proof Call Jack Station



UL 1069 and CSA C22.2#205
5002971

BENEFITS

- Reliable Signaling
- No Maintenance
- Low Power
- Simple Wiring
- Easily Integrates to other Systems
- Attractive Station Hardware

The Tech Works **NC-VP-PBS** is a call for HELP Station with a ¼ inch call cord jack and a Vandal Resistant Push button with concentric Call Assurance Light built in to the button and mounted on a rugged stainless-steel plate. The call cord jack is provided for activating the Normal or Bed Call directly at the station. Call cancel is a Lighted Button to reset the station. The reset can be either local or a remote key switch or a remote lighted push button.

An integral call confirmation LED notifies the user that a call has been sent. The Call Assurance Light will be Off if no call is pending, glowing steadily if a Normal Call is pending, and flashing if an Emergency Call is pending.

This is a passive button and light assembly designed for use with active stations like the **NC-DL-12-R** Dome Light. Screw Terminals provide wiring connection to the active electronic stations that provide signaling and control for the **NC-VP-PBS**.

Mounting is a standard 1-gang electrical box. The Face Plate is made of 12-gauge Stainless Steel with a brushed finished and includes tamper resistant mounting screws.

Associated Equipment

PBC-7	Push Button Cord 7 ft.
NC-DL-12	Dome Light
VPKS-1	Vandal Proof Key Switch
VPBL-1	Vandal Proof Button/Lite

Design Information

Power	15V DC
Color	Stainless Steel
Mounting	1 Gang Back Box
Dimensions	3.25" W x 0.5" D x 5" H
Weight	1 lb.

Architects' and Engineers' Specifications

The Nurse Call System Patient Bed Station shall be a standard one gang electrical box mounting device constructed of Vandal Resistant Stainless Steel. A ¼ inch phone jack shall be included to place a Patient Bed Call to the System. A remote Cancel button shall be provided to reset the station. A call confirmation light shall be included to indicate that a call has been placed. The staff station shall be a passive electronic device requiring no more than 3 mA at 15 Volts DC for full operation.

The Nurse Call System Patient Bed Station shall be Tech Works Model NC- VP- PBS




Tech Works®

"Making Specialized Communication Easy"



Quick Start Installation Instructions

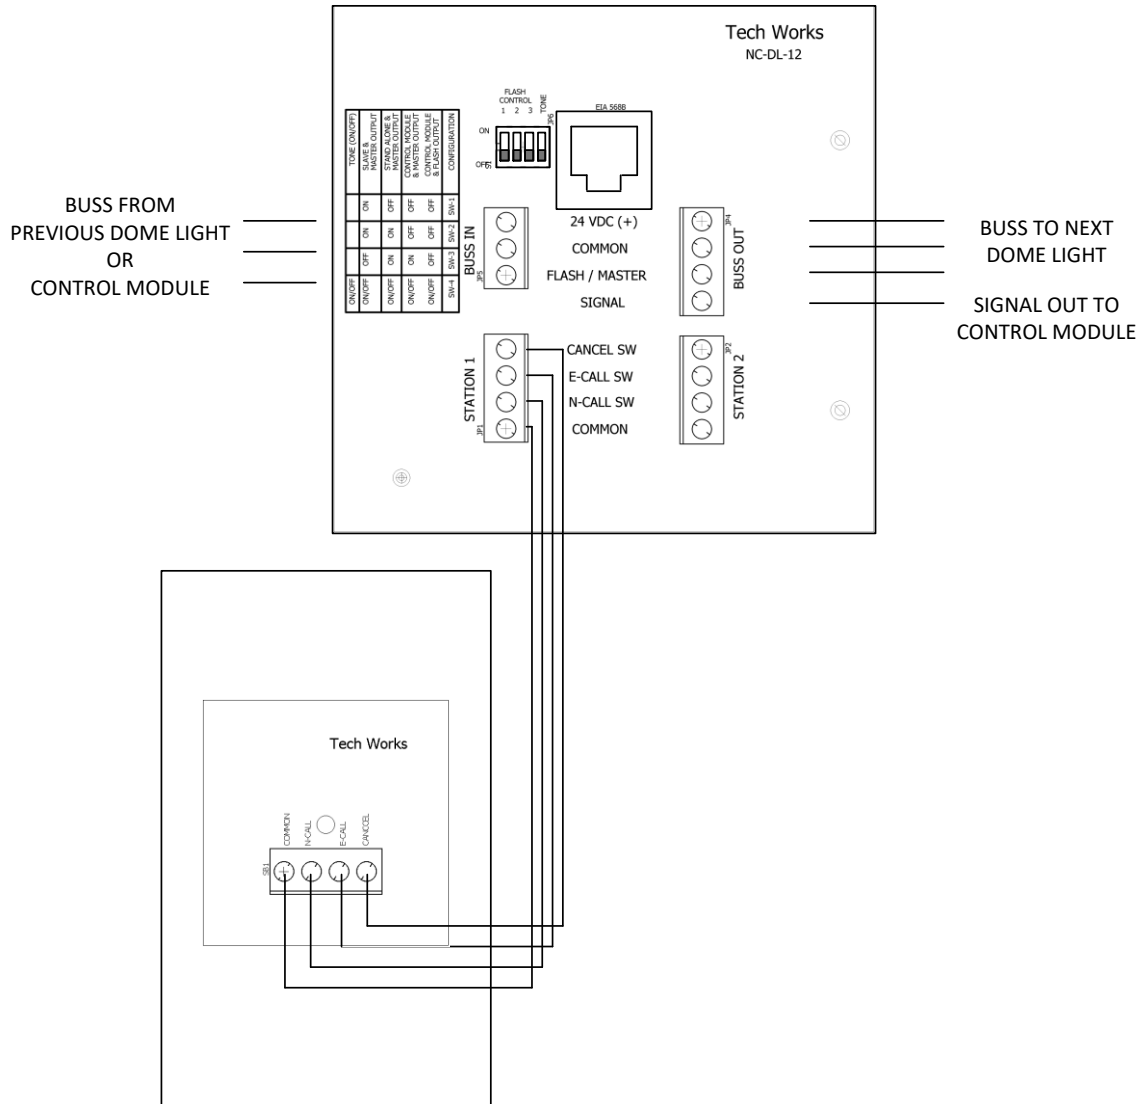

For further system set up and adjustment please see the System Planning Guide by scanning the QR Code.

